



Mod. 60

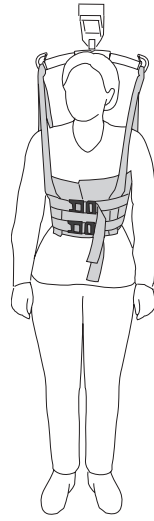

Mod. 64

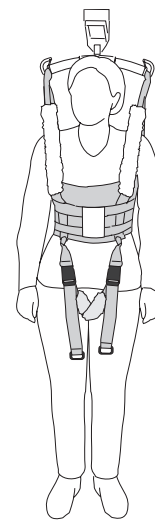

Mod. 60
with leg harness
and padded cases

Product Description

This instruction guide is valid for Liko MasterVest and "TeddyVest", but in the following text we will only use the name Liko MasterVest.

Liko MasterVest is a versatile sling with a wide range of uses, for example, help with standing and walking or visiting the toilet.

MasterVest supports the patient around the upper body as well as under the arms. MasterVest requires patients to be able to partially weight bear.

Liko MasterVest enables you to reach certain difficult-to-achieve goals, for example:

- patients receive appropriate help to exercise and bear weight on their legs, and
- caregivers avoid risks associated with heavy lifting.

Lifting and transferring patients to and from the toilet can lead to severe injuries for the caregiver.

MasterVest facilitates smooth and simple transfers to and from the toilet.

Since MasterVest covers only the upper body, the lower body is easily accessible for dressing and undressing.

Liko MasterVest in sizes XXS and XS are made of a Teddy bear patterned polyester fabric and this is why these slings are called "TeddyVest".

Front closure MasterVest, Mod. 64

The front closure model of Liko MasterVest Mod. 64 can be used for patients who are able to put on and take off the vest by themselves.

The front closure MasterVest is equipped with two adjustable safety clasps across the chest.

These are also recommended in cases where it is necessary to adjust the tension and regulate pressure on the chest.

Front closure MasterVest in size XS is made of a Teddy bear patterned polyester fabric and this is why this sling is called "TeddyVest", front closure.

MasterVest with Leg Harness


The leg harness holds MasterVest in place and is commonly used in walking training.

△ "Caution!" triangles are used to warn of situations that demand extra care and attention.


In this document, the person being lifted is referred to as the "patient" and the person helping them is referred to as the "caregiver".

 Before using lifts and lifting accessories, read the instructions for both the sling and the lift that will be used. Instruction guides can be downloaded, free of charge, at www.liko.com.

Liko MasterVest

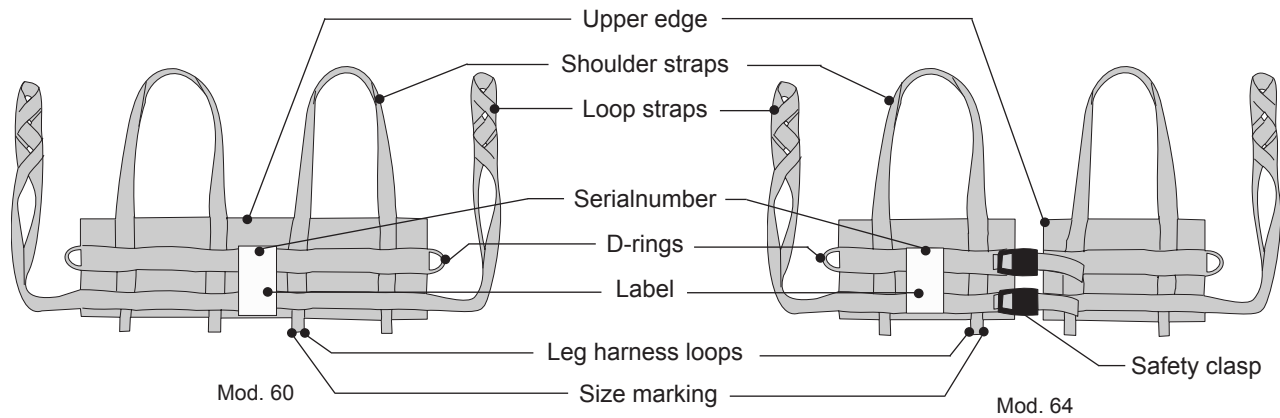

Lifting from a seated position

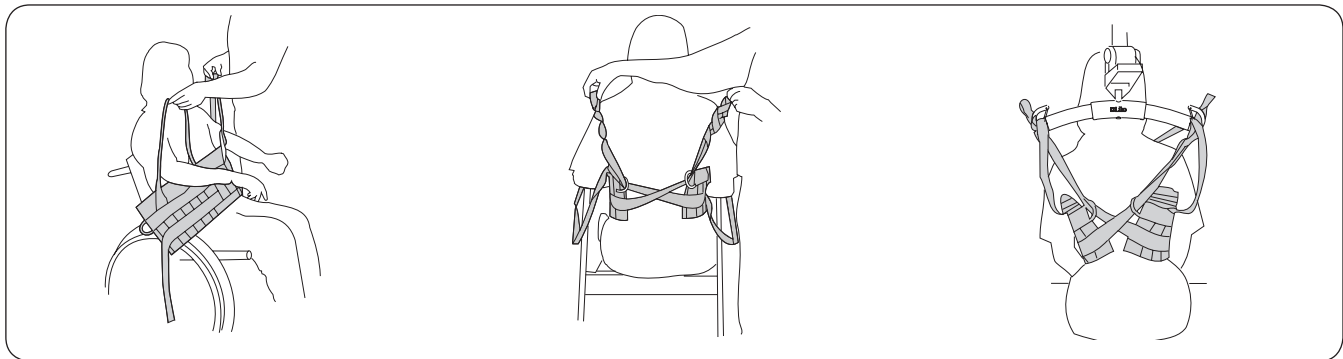

Put on MasterVest from the front. The patient's arms are placed through the shoulder straps.

Behind the back: Draw each loop strap across the back and pull it through the metal D-ring on the opposite side, as shown in the illustration.

With the slingbar behind the patient's back, attach the loop straps, using a suitable loop, see page 3. Attach the shoulder straps to the slingbar.



Before lifting: Check that the patient's feet are solidly on the floor so that he/she can bear weight as the slingbar is raised. Raise the slingbar slightly to tighten the straps (without lifting the patient off the seat), and check that the pressure distribution around the patients upper body feels correct.


During the lift: Pull the slingbar forward so the patient's weight is transferred smoothly until he/she stands upright and in balance. Lower the slingbar slightly to relieve pressure around the chest. Now the patient has an opportunity to put weight on the legs and work on balance training.

Testing the Liko MasterVest

Selecting the right size

For MasterVest to function properly, the width of the vest must be in correct proportion to the circumference of the patient's upper body.

Therefore, it is important to select the right size and carefully determine the correct loop on the loop strap.

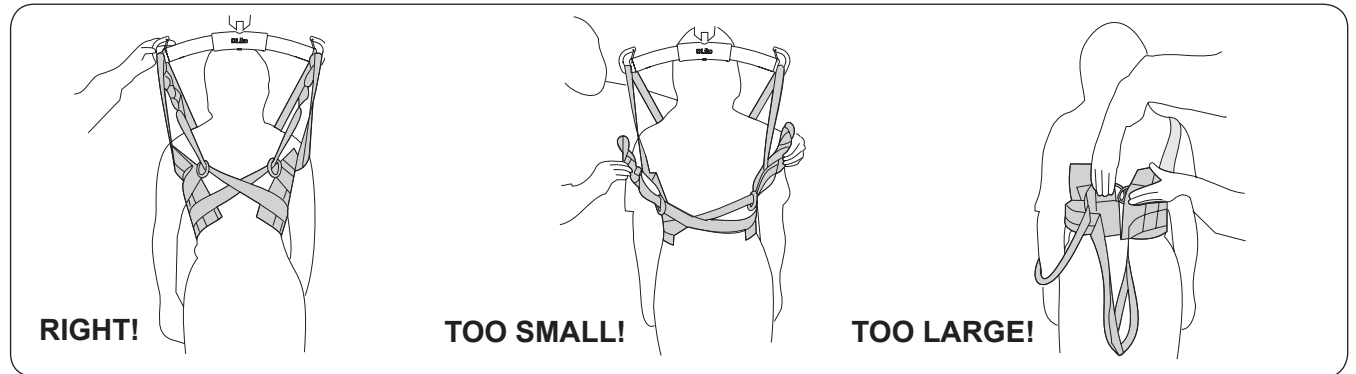

RIGHT!
The size is right when the gap between the metal D-rings is between 5 cm (2 inch.) and 30 cm (11.8 inch.). The larger the size of the vest, the wider the gap can be.

TOO SMALL!
The size is too small when the gap between the metal D-rings is too wide, the loop straps do not reach up to the slingbar, and the pressure around the chest is too great.

TOO LARGE!
The size is too large when the metal D-rings touch. The vest is too wide and does not tighten during lifting but slides upward. A vest that is too large creates too much pressure under the armpits.

Adjusting the Loop Straps


The loop which you hook onto the slingbar determines how much the vest tightens around the chest.

If the vest slides upward - try an inner loop or a smaller size of the vest.

If the vest fits too tightly around the chest - try an outer loop or a larger vest size.

If two different people try the same size, the slimmer person would need an inner loop while a bigger person would need an outer loop. The MasterVest is correctly adjusted when the shoulder straps and loop straps are equally taut when lifting the patient.

Testing the Loop Straps

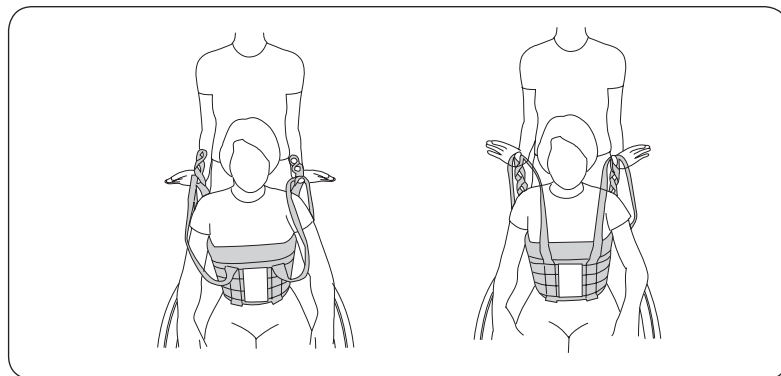


To find which loops give the best fitting, test the loop straps by drawing on different loops along with the shoulder straps.

To test for the correct fitting of the loop straps, stand behind the patient and suspend the shoulder straps and loop straps from your thumbs and lift upward until the straps are taut.

The MasterVest fits correctly when the loop straps and shoulder straps are equally taut when lifted.

Body posture

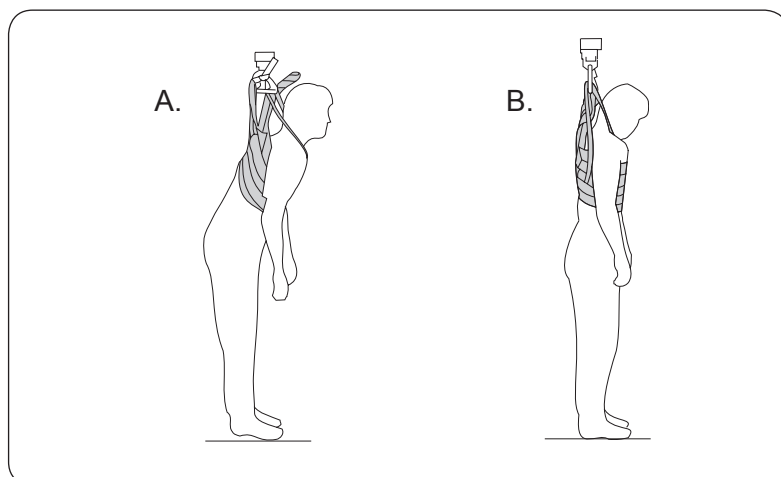

An individual may often fit into two different sizes of the MasterVest, but the loop straps must be correctly adjusted to each size.


The results differ regarding body posture and pressure distribution around the chest.

A. A larger MasterVest size requires you to use one of the inner loops on the loop strap. This fitting allows the patient to bend forward, and places more pressure on the lower front part of the chest.

B. A smaller MasterVest size requires you to attach one of the outer loops of the loop strap to the slingbar to obtain equal tension on all four straps. In this case, body posture is more upright and pressure is more evenly distributed around the chest.

Liko MasterVest accessories


Leg Harness

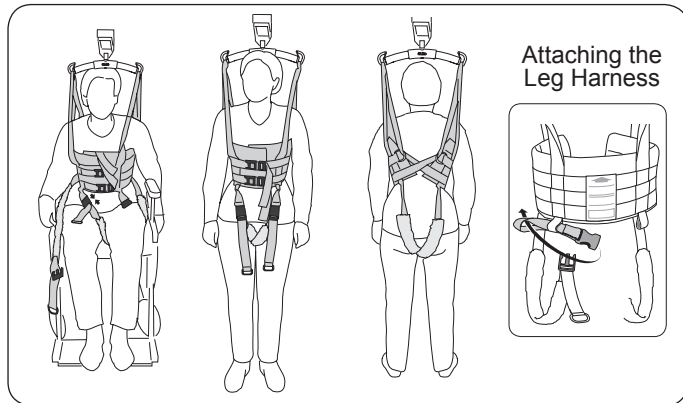

A special leg harness can be used with the Liko MasterVest to help keep the vest from sliding up on the body.


The harness can be put on while the patient is sitting, and after lifting the patient you can adjust the position and tension of the harness.

The harness straps may be crossed or parallel through the crotch.



Loop Clips

This practical accessory is used to mark the loops that have been tried out for a certain person. It makes it easier for the caregivers to choose the right loop to attach to the slingbar.

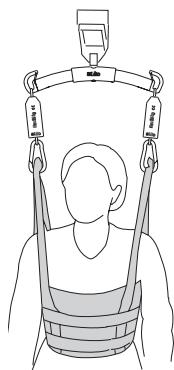

Springs

Springs are available as an accessory in order to enable a gentler, springy motion during gait training. They stimulate the natural pattern of movement and allow the patient to find the right walking technique.


Liko's Springs for patient weights up to 70 kg (154 lbs.) are available in two lengths:

- Long 28 cm (11 inch.), Prod. No. 3156511 and
- Short 22 cm (8.7 inch.), Prod. No. 3156512

Short springs are recommended in cases where the lifting height does not permit the use of long springs.

For patient weights up to 100 kg (220 lbs.):

- Short 22 cm (8.7 inch.), Prod. No. 3156513

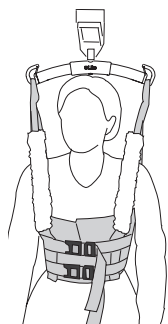

Padded Cases

Padded cases are available as an accessory to help relieve pressure on the front shoulder straps.

Padded cases are equipped with Velcro along one side for easy application.

△ Before lifting, remember the following!

- The need for one or more caregivers must be determined from case to case.
- Plan the lift carefully to ensure that it is performed as safely and conveniently as possible.
- Although Liko's slingbars are equipped with safety latches, particular care must be taken. Before the patient is lifted from the underlying surface, but after the straps have been fully extended, make sure the straps are properly hooked to the slingbar.
- Never lift a patient higher above the underlying surface than is necessary for the lifting and transfer procedure.
- Never leave a patient unattended during a lifting situation.
- Make sure the wheels on the wheelchair, bed, gurney, etc. are locked during the lifting/transfer operation.

Caution!

Test the emergency lowering device on the lift you are using to make certain that it functions properly. Adjust the maximum height so that it will be impossible to raise a patient too high.


Problem during testing?

Problem: The vest slides up under the patient's arms.

Adjust the MasterVest using one or more of the following suggestions:

- Adjust the loop strap by using an inner loop.
- Choose a smaller size.
- Try using a Liko MasterVest of plastic-coated net.
- Try using the leg harness (see page 4).
- Hold the vest in place behind the back while raising the patient by pressing your thumb downward on the crossed loop straps.
- Have the patient keep his/her arms down while lifting.

Front closure MasterVest, Mod. 64

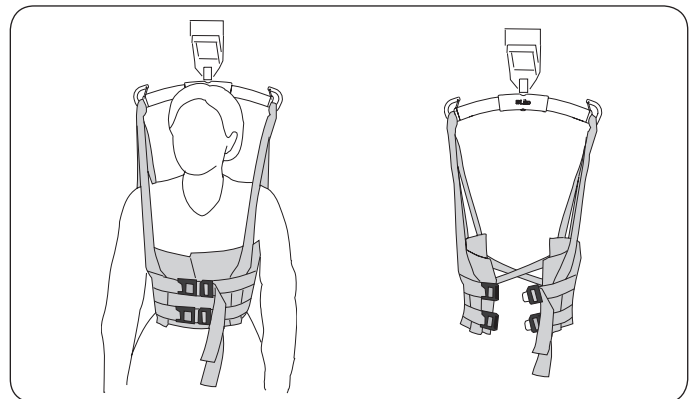


The MasterVest is also available in a front closure model. The front closure MasterVest is equipped with two adjustable safety clasps in front. Test for the correct vest size and position of the loop straps even when patients themselves put on the MasterVest. After the MasterVest has been correctly adjusted, it can hang from the slingbar while the patient puts it on.

Liko MasterVest in plastic-coated net


The most common sizes of the MasterVest are available in plastic-coated net. Friction from the material counteracts the tendency of the vest to slide upward.

A MasterVest in plastic-coated net may also be used for bathing.

Overview Liko MasterVest, Mod. 60, 64



Mod. 60



Mod. 64

Product	Prod. No.	Prod. No.	Size	Body Weight kg*	Maximum load
"TeddyVest"	3560812		XXS	< 20 kg (< 44 lbs.)	200 kg (440 lbs.)
"TeddyVest"	3560813	3564813	XS	20-40 kg (44-88 lbs.)	200 kg (440 lbs.)
MasterVest	3560 - 14	3564 - 14	S	40-60 kg (88-132 lbs.)	200 kg (440 lbs.)
MasterVest	3560 - 15	3564 - 15	M	60-80 kg (132-176 lbs.)	200 kg (440 lbs.)
MasterVest	3560 - 16	3564 - 16	L	80-100 kg (176-220 lbs.)	200 kg (440 lbs.)
MasterVest	3560 - 17	3564 - 17	XL	100-130 kg (220-286 lbs.)	300 kg (660 lbs.)
MasterVest	3560 - 18		XXL	120- kg (264- lbs.)	300 kg (660 lbs.)

* NOTE! The body weights given are general recommendations only. Variations are normal.

		<u>Light green</u>	<u>Dark green</u>	NOTE! The leg harness fits vests from serial number 736166. Contact Liko for information on earlier models.
Leg Harness, pair	XS, S	3666004	3666007	
Leg Harness, pair	M, L	3666005	3666008	
Leg Harness, pair	XL	3666006	3666009	

356 - - 16 → Size

1 Polyester 4 Plastic-coated net (can be wiped clean and disinfected with alcohol) 8 Teddy bear patterned polyester

0 Liko MasterVest
4 Liko MasterVest, front closure

Order number example: Prod. No. 3560115
Liko MasterVest, Polyester, Medium.

Laundering: See the sling's product label.

Expected Life Time

The product has an expected life time of 1-5 years with normal use. Expected life time varies depending on the fabric, use frequency, washing procedure, and weight carried.

Periodic Inspection

The product must be inspected at least once every 6 months. More frequent inspections might be required if the product is used or washed more often than normal. See Liko's protocol Periodic Inspection for the respective product.

Recommended combinations using Liko MasterVest with Liko slingbars:

	Mini 220	Slim 350	Universal 350	Standard 450	Universal 450	Wide 670	Twinbar 670
"TeddyVest", XXS	1	1	1	2	2	4	4
"TeddyVest", XS	1	1	1	2	1	4	4
MasterVest, S	2	1	1	1	1	2	2
MasterVest, M	2	1	1	1	1	1	2
MasterVest, L	2	1	1	1	1	1	1
MasterVest, XL	3	2	1	1	1	1	1
MasterVest, XXL	3	3	2	1	1	1	1

Code:

- 1 Recommended
- 2 Possible
- 3 Not advisable
- 4 Inappropriate

The above table gives several recommendations for each size. Different slingbar widths create different levels of pressure on the chest. Try various alternatives until you find the one best suited to the individual patient. Combinations with Liko MasterVest and Cross-bar, Cross-bar 450/670 or Side bars is not appropriate.

CE Class I medical-technical product

Liko MasterVest has been tested by an accredited testing institute and complies with all requirements for MDD Class I products and the harmonized EN ISO 10535 standard.

Liko's products are constantly being updated and refined. Liko reserve the right to change aspects of the products without prior notice. Contact your local Liko representative for updated information and advice.

⚠ Important!

Lifting and transferring a patient always involves a degree of risk. Study the instruction guides for both lift systems and accessories carefully. A complete understanding of the contents of instruction guides is essential.

Only trained personnel should use the equipment.

Make certain that the lift accessories are appropriate for the lift you are using and for the lifting situation. Exercise caution and care when using lift equipment and accessories.

As a caregiver, you are responsible for the patient's safety. You must be well informed of the patient's condition and ability to manage the lifting situation.

Inspect the sling regularly, especially after laundering. Check carefully for wear and damage to seams, fabric, straps and strap loops. Never use damaged accessories! When in doubt, contact the manufacturer or supplier.



A Hill-Rom Company

www.liko.com

Manufacturer:

Liko AB
SE-975 92 Luleå
Sweden
info@liko.se

